





Scanning Laser Ophthalmoscope

# Mirante

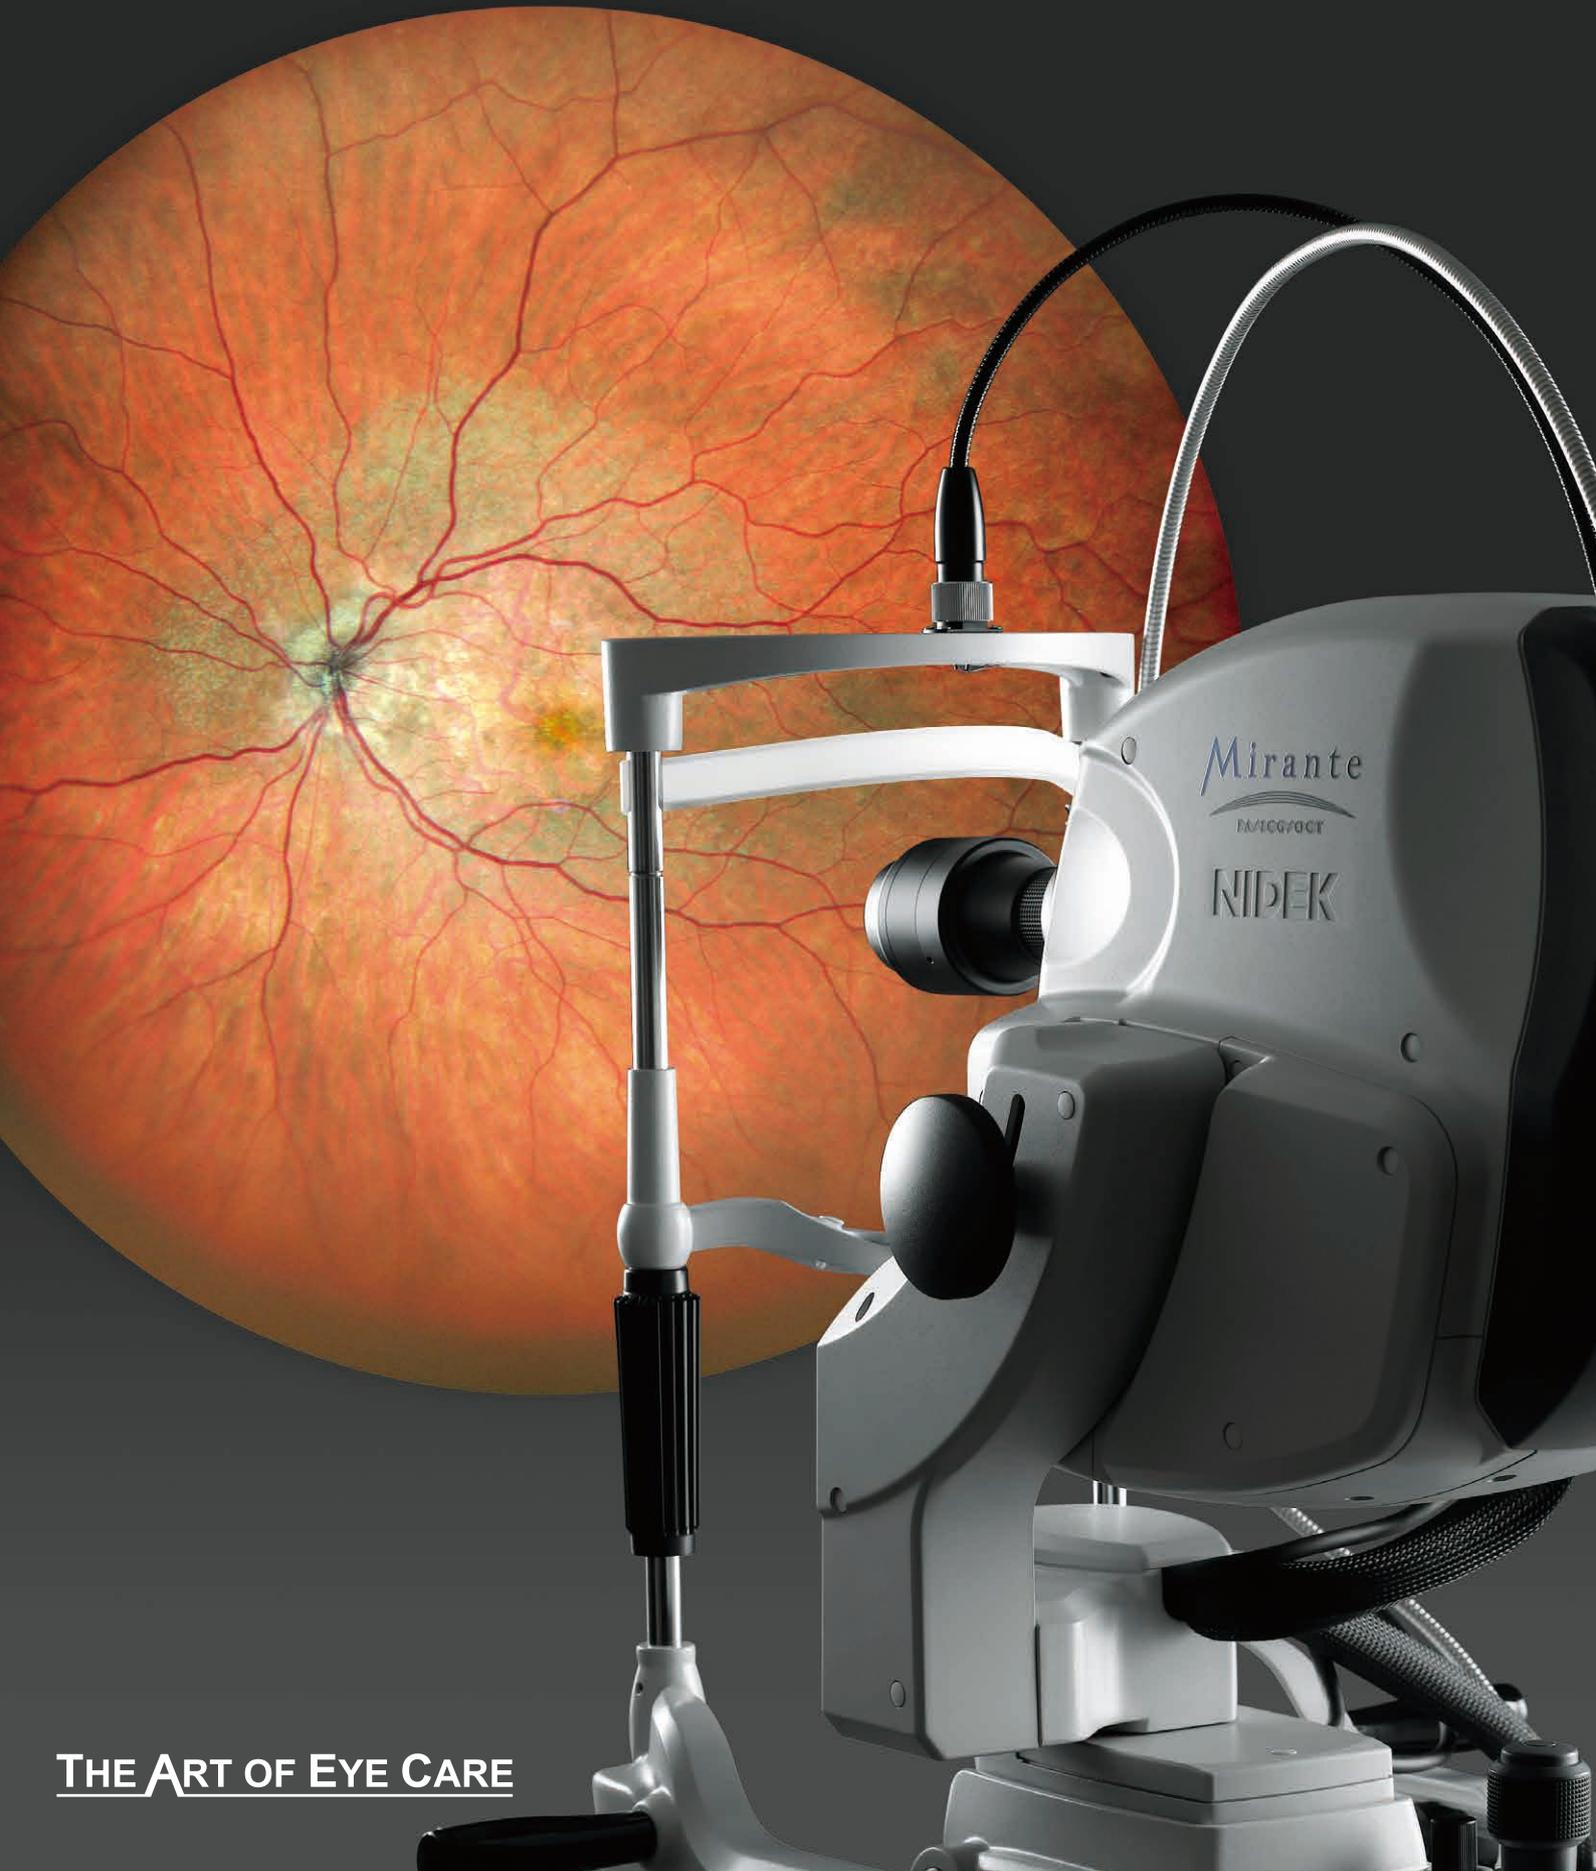

THE ART OF EYE CARE

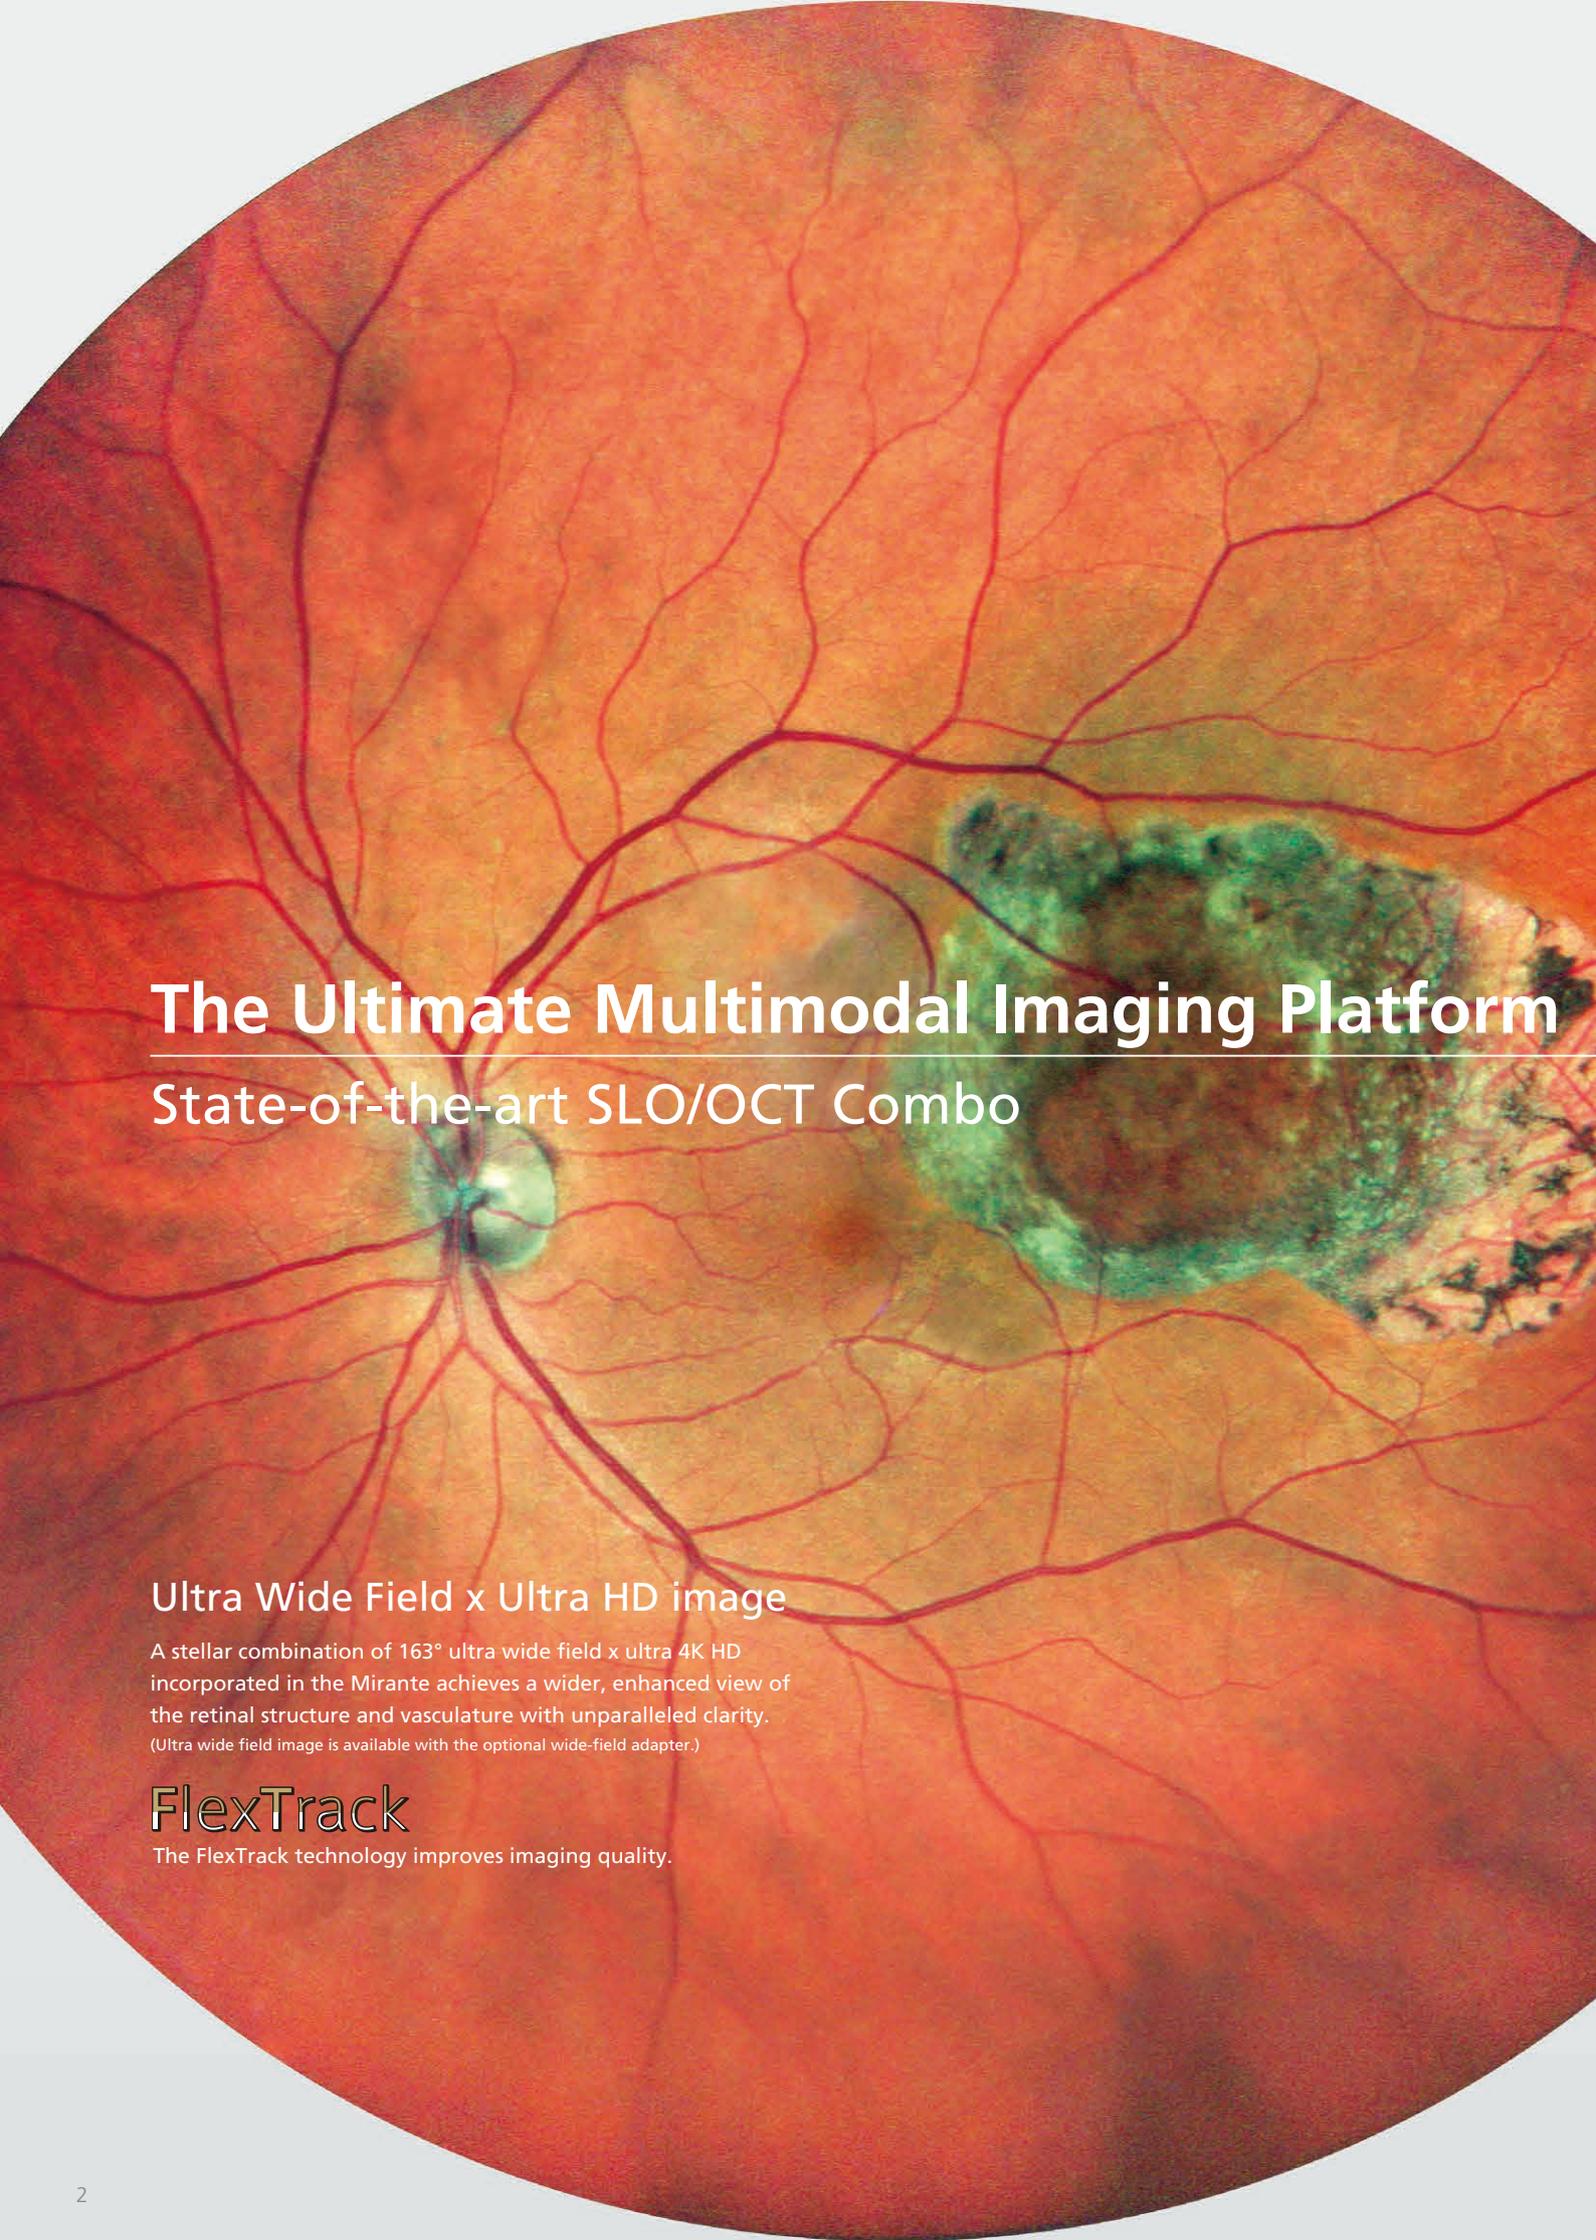

# The Ultimate Multimodal Imaging Platform

---

## State-of-the-art SLO/OCT Combo


### Ultra Wide Field x Ultra HD image

A stellar combination of 163° ultra wide field x ultra 4K HD incorporated in the Mirante achieves a wider, enhanced view of the retinal structure and vasculature with unparalleled clarity.






(Ultra wide field image is available with the optional wide-field adapter.)

### FlexTrack


The FlexTrack technology improves imaging quality.

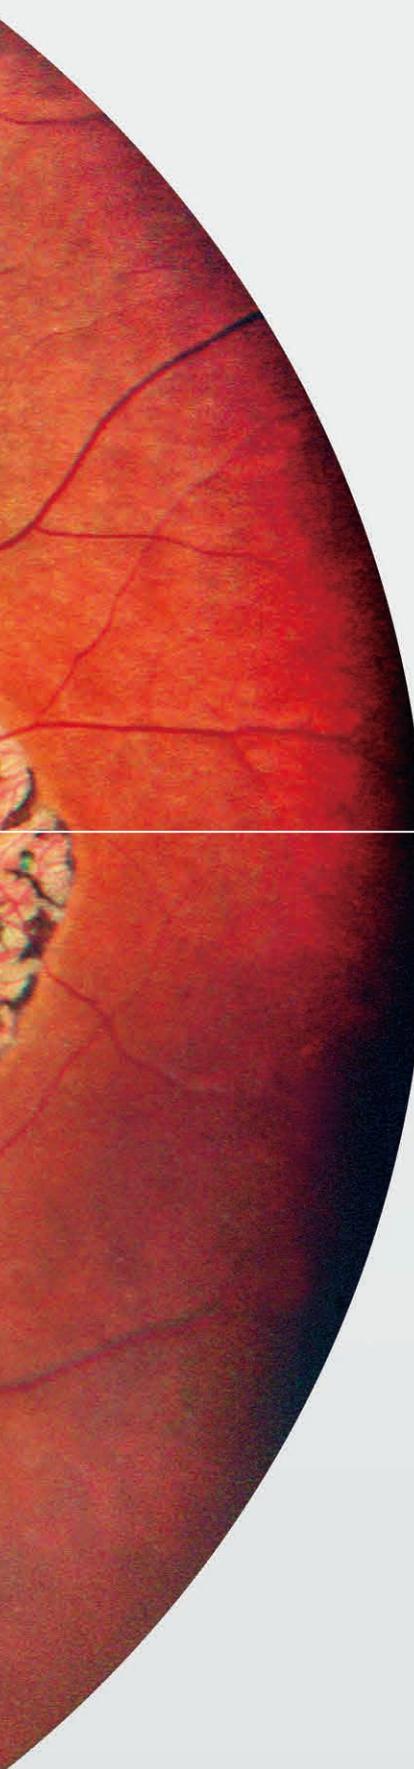

## Confocal SLO

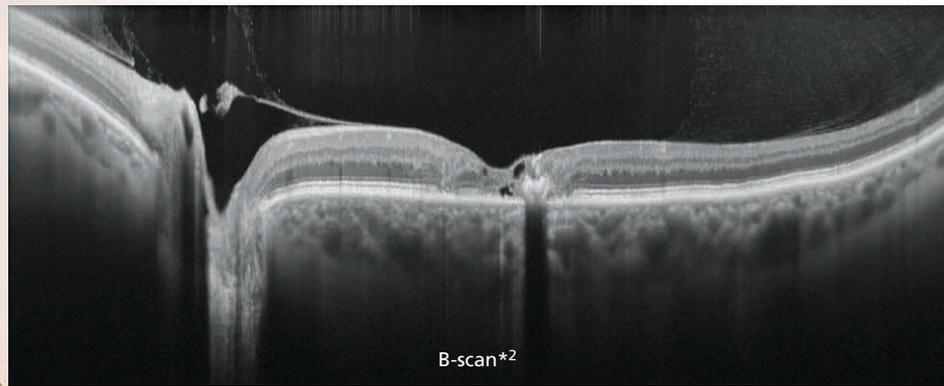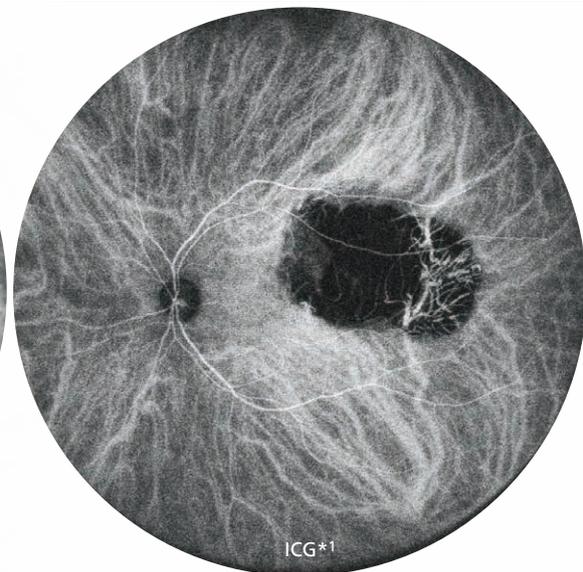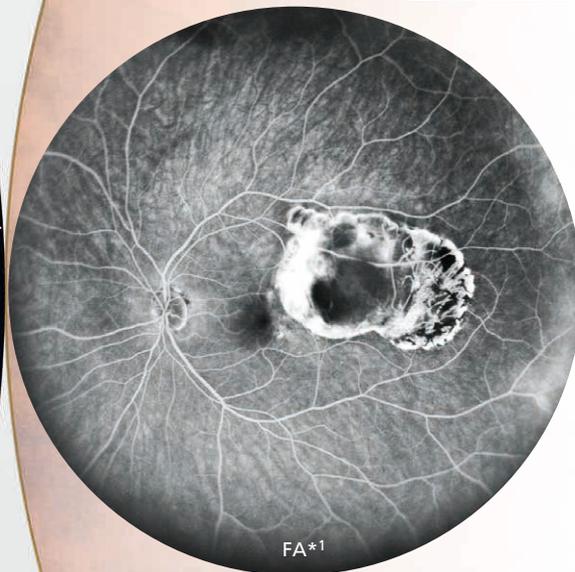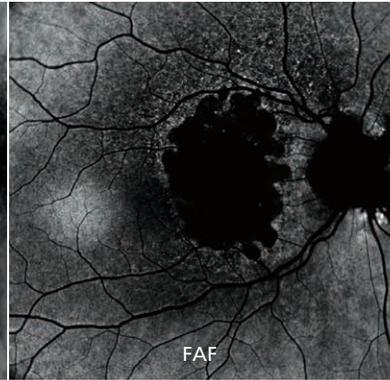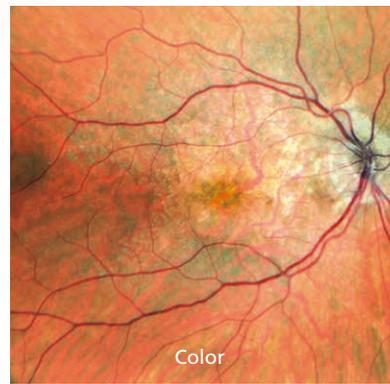

## OCT

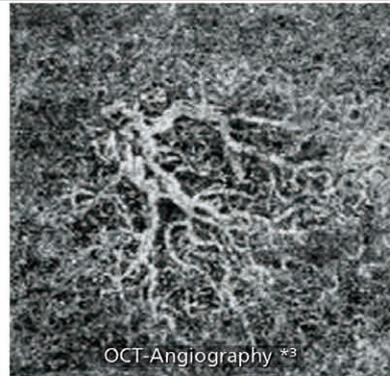

\*1 Available for the SLO/OCT model. Optional for the SLO model.  
\*2 Available for the SLO/OCT model.  
\*3 Optional for the SLO/OCT model.

**163° ultra wide field color image**

The clear image of the entire 163° field of view enables detailed evaluation of pathologies from the fovea to the extreme periphery.

(Ultra wide field imaging is available with the optional wide-field adapter.)

**Refine mode**

As required, capturing two images with slightly different fixation reduces reflection, producing a clear ultra wide field image.



89° standard color image

163° ultra wide field color image

**Panorama image composition**

Panorama imaging with preset fixation points captures details of pathology even in the extreme periphery.



Panorama image

**Tilt and swing features**


The tilt and swing functions for the optical head allows imaging of the peripheral fundus and acquisition of panorama images. These functions also help for patients with unstable fixation.



Tilt




Swing

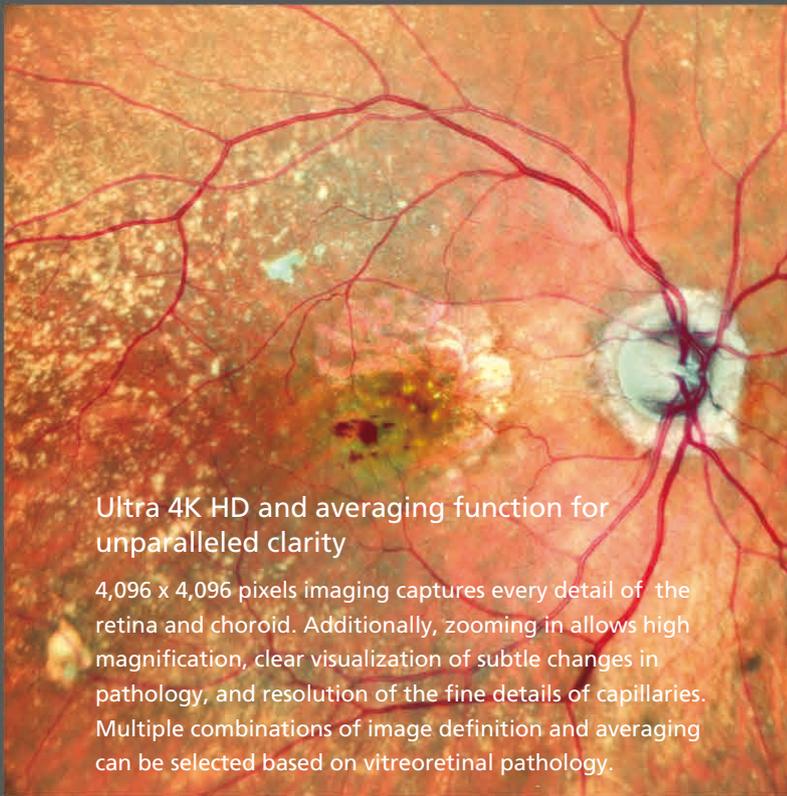

**Ultra 4K HD and averaging function for unparalleled clarity**  
 4,096 x 4,096 pixels imaging captures every detail of the retina and choroid. Additionally, zooming in allows high magnification, clear visualization of subtle changes in pathology, and resolution of the fine details of capillaries. Multiple combinations of image definition and averaging can be selected based on vitreoretinal pathology.


## FlexTrack

The FlexTrack algorithm corrects image distortion due to unstable fixation and enhances averaging quality.

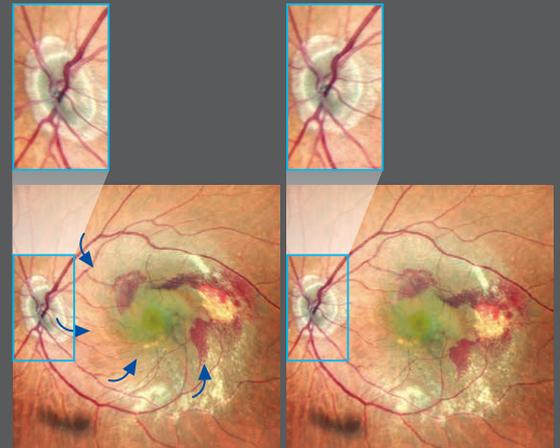


Distorted image due to poor fixation

Corrected image using FlexTrack

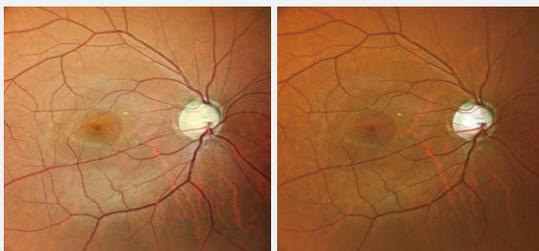


Color histogram adjusted similar to slit lamp view

Color histogram adjusted similar to fundus camera image



## RGB triple detectors

Three separate RGB detectors simultaneously scan different depths of retina with red, green, and blue wavelengths. A color histogram is available for fine adjustment based on pathology or practitioner preference.

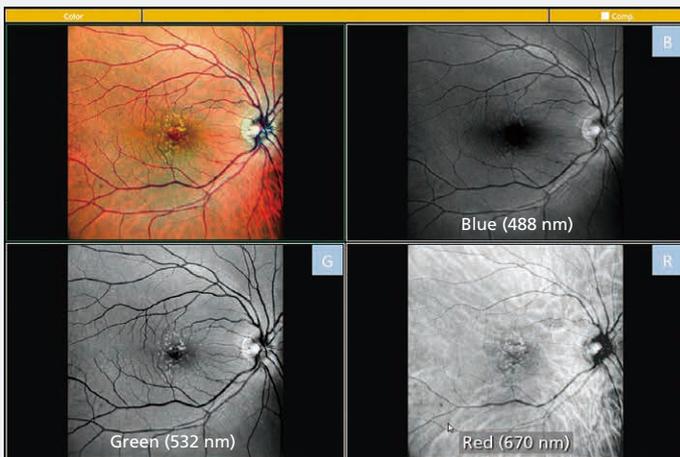

Summary view for RGB color and single color images

## RGB color + selectable color display with a single shot


Single color images in red, green, and blue wavelengths can be displayed after color image acquisition. Each wavelength is available with just a single shot, and the image layers can be selected based on user preference or a specific pathology. The viewer software allows image processing options including noise removal and adjustments for brightness, contrast, and sharpness.




### Retro mode

Retro mode is a unique non-invasive technique for detecting pathologic changes in the choroid.

This imaging modality uses scattered IR light to detect abnormal reflection in the choroid caused by drusen, edema and other subtle chorioretinal pathologies.

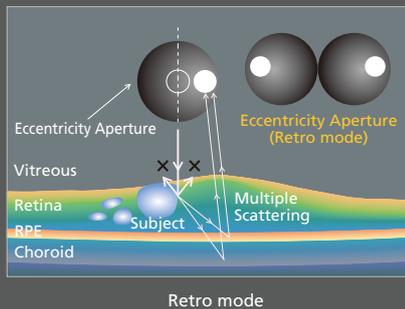


### Drusen

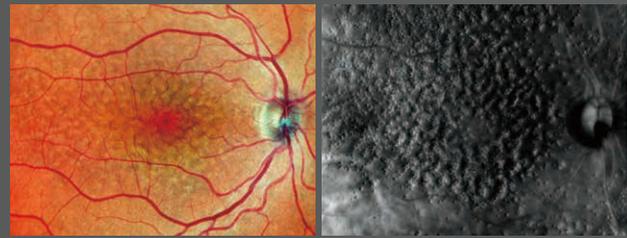

Color

Retro mode


### Stargardt disease

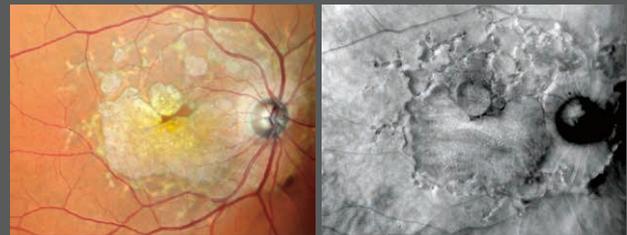

Color

Retro mode

### CNV

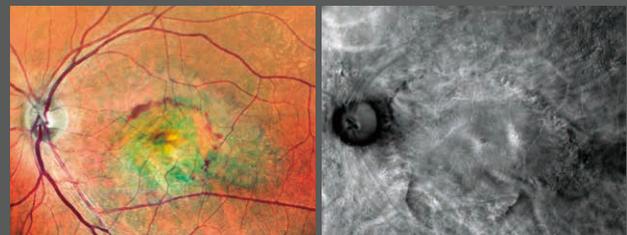

Color

Retro mode

### Blue-FAF / Green-FAF (fundus autofluorescence)


FAF imaging is a non-invasive method to evaluate the retinal pigment epithelium (RPE) without contrast dye.

Green-FAF reduces the effects of xanthophyll from the macula on imaging and is useful for monitoring deeper layers under the macula.

Blue-FAF imaging captures high definition images for diagnosing early AMD.

Gain level and contrast can be adjusted manually or automatically depending on the vitreoretinal pathology.


### Geographic atrophy

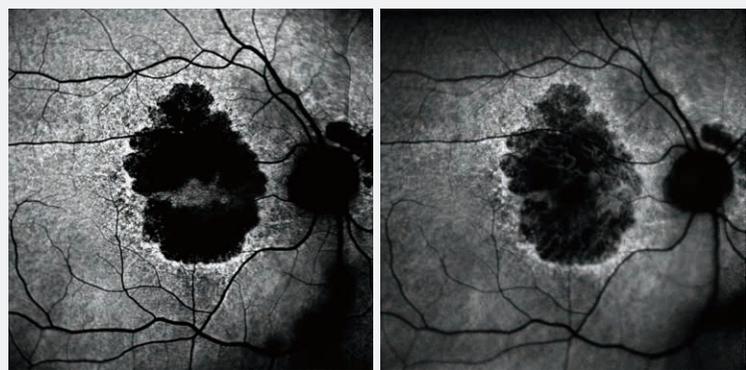

Green-FAF

Blue-FAF

### Macular dystrophy

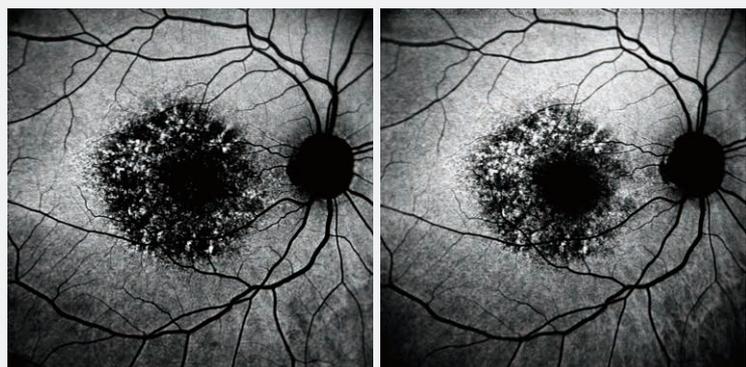

Green-FAF

Blue-FAF




### Simple interface and easy operation

The Mirante has multiple modalities and functions with interface software that presents these choices in a simple, easy-to-use manner. Image acquisition with the Mirante is simple. The SLO image is focused automatically by pressing the optimize button. After optimization is completed, the image can be captured by pressing the release button.

Presenting multimodal images in a summary screen allows faster, more comprehensive evaluation of disease.


### Streamlined combination capture

The Combo image capture allows sequential capture of images with the preset combination of image capture settings for each specified disease.

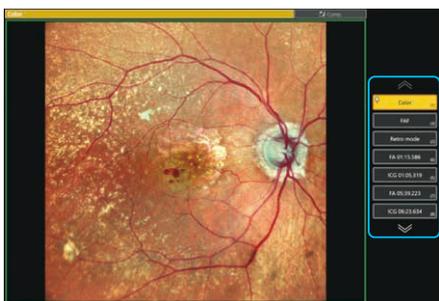


### Fly Through

The Fly Through function further enhances multimodal imaging by registering and synchronizing images from different modalities to view the same area while scrolling through the region of interest.

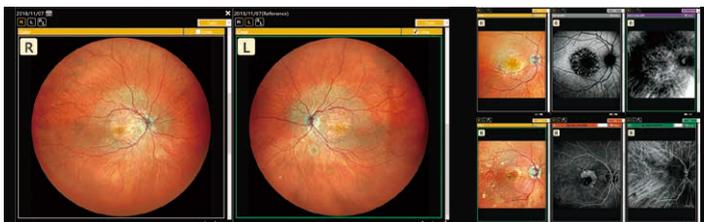

### Side by Side

The Side by Side function displays up to 3 images on one screen for all SLO modalities for the left and right eyes and displays the images in chronological order.

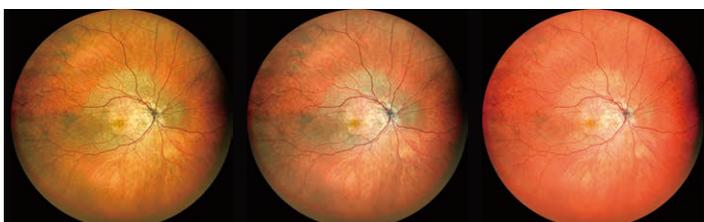

### Image processing preset

Image processing parameter settings allow the clinician to easily display images in the preferred retinal color.



### 163° ultra wide field FA and ICG images

(Ultra wide field imaging is available with the optional wide-field adapter.)




163° ultra wide field FA image



163° ultra wide field ICG image



89° standard FA image

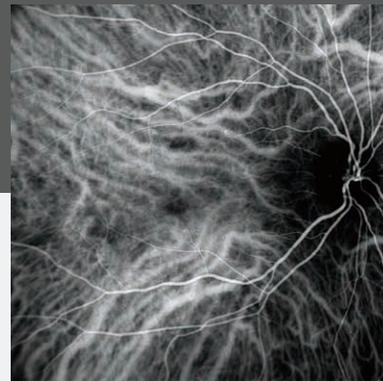

89° standard ICG image


### HD dynamic and static angiogram

Auto gain control (AGC) optimizes gain levels and contrast for early, peak, and late phase angiography.


High definition imaging up to 16 megapixels, can be selected based on ocular pathology. The averaging function for static and dynamic imaging ensures high contrast even during late phase angiography while simultaneously reducing noise on images and video.

Videos can be recorded at a maximum of 1,024 x 1,024 pixels for up to 120 seconds. Multiple short videos can be recorded during the same measurement.


FA



Early phase







Mid phase



Late phase

ICG



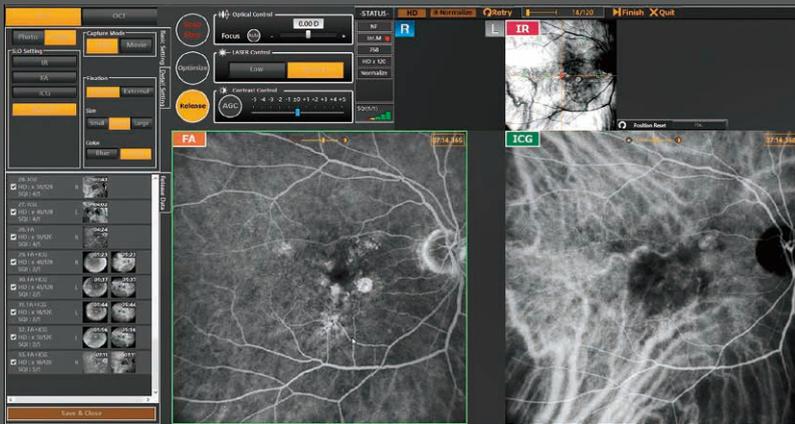

Simultaneous FA and ICG imaging display (standard)



Simultaneous FA and ICG imaging display (ultra wide field)

## Simultaneous FA and ICG

The Mirante allows simple, simultaneous acquisition of FA and ICG images. The live IR monitoring enables alignment prior to fluorescence emission and reduces the risk of missing the very early phase of angiography. The AGC simultaneously adjusts contrast of each FA and ICG image, making the imaging of dynamic blood flow a very simple procedure.



Live IR monitoring

Using live IR monitoring, physicians can start alignment before fluorescence emission.

## Easy comparison of FA and ICG


The viewer software can present FA and ICG images side-by-side, facilitating convenient and comprehensive evaluation of angiography.




Side-by-side display of FA and ICG

## FA and peripheral fundus

The tilt and swing features and ultra wide field capability allows peripheral imaging during fluorescein angiography.

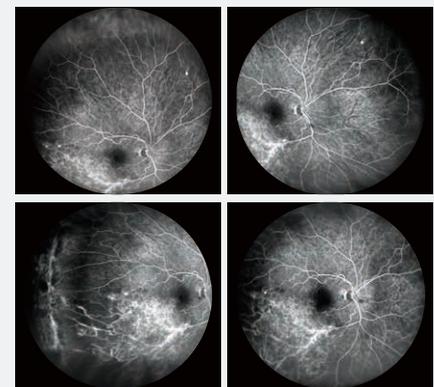


FA of the peripheral fundus

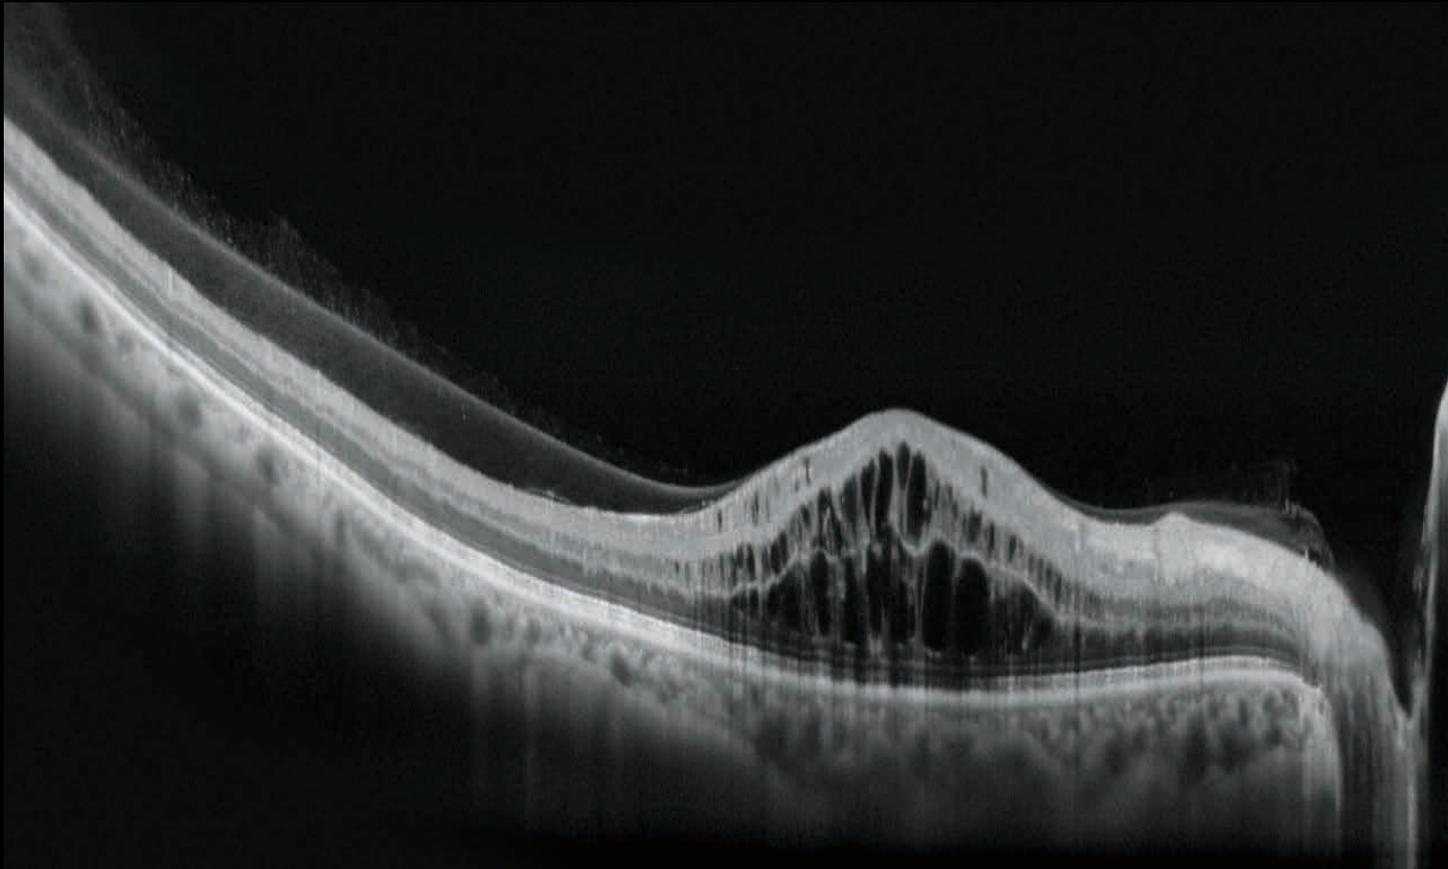

Macula line 16.5 mm / 2,048 A-scans

### HD wide area OCT

The maximum 16.5 x 12 mm area scan available with the Mirante allows wide area diagnosis including the macula and optic disc in a single shot. The ultra fine mode and tracing HD plus functions provide high quality images for detailed observation from the vitreous layers to the choroid.

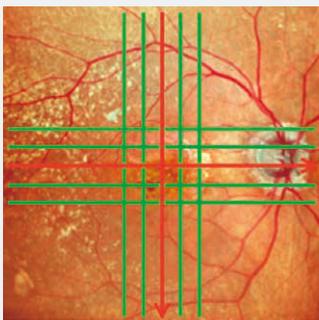


SLO image




Macula multi cross 12 x 12 mm




Retina map  
12 x 9 mm  
1,024 A-scans x 128 lines

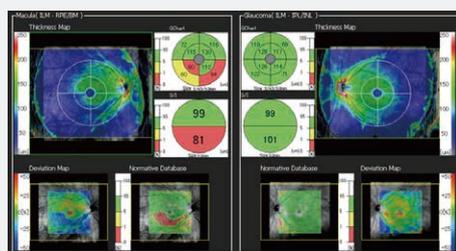

Macula map (both eyes)

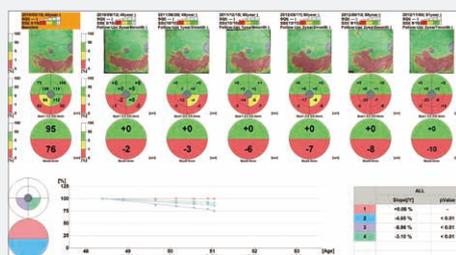

Glaucoma follow-up

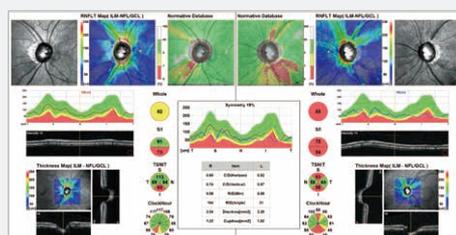

Disc map (both eyes)

## Glaucoma analysis

The Mirante incorporates 16.5 x 12 mm thickness map which visually presents pathological changes from the central retina to the periphery.



9 x 9 mm normative database allows [NFL+GCL+IPL] analysis from optic disc to macula in a single report.

### Segmentation into multiple slabs

The simple interface provides seven slabs for the macula map / four slabs for the disc map with intuitive functionality and removal of projection artifacts.

### Follow-up function

The follow-up function presents the changes over time, in vessel density or perfusion density in easily understandable maps. Data are presented in chronologic order to evaluate vascular changes with disease progression.

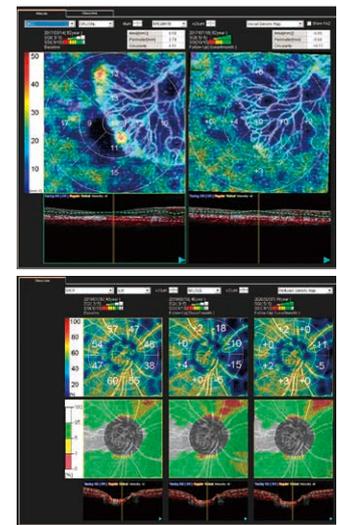
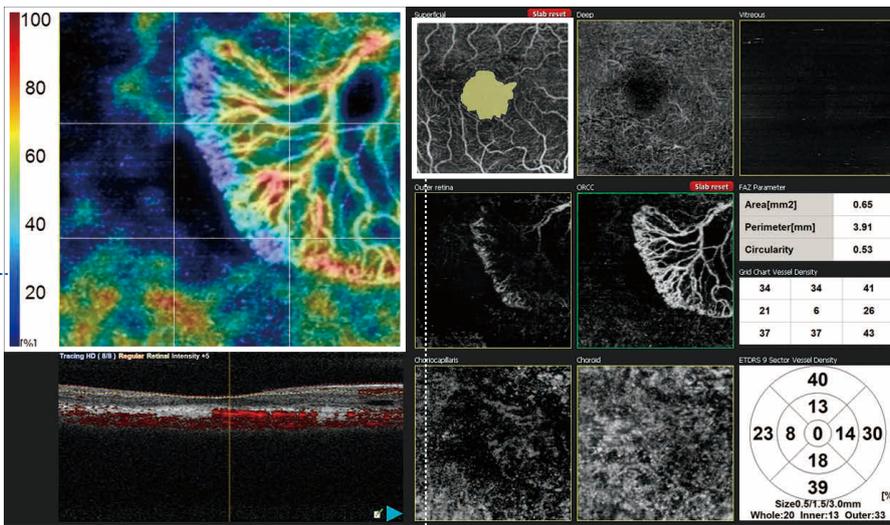


### Vessel Density Map and Perfusion Density Map

Quantification of vessels in each layer provides metrics to assess disease progression and the effects of treatment. Quantitative analysis can be performed with the Vessel Density Map and Perfusion Density Map. Both maps can be displayed in all slabs.


### Autodetection of FAZ and shape analysis

Foveal Avascular Zone (FAZ) is automatically detected and shape metrics are provided for rapid assessment.

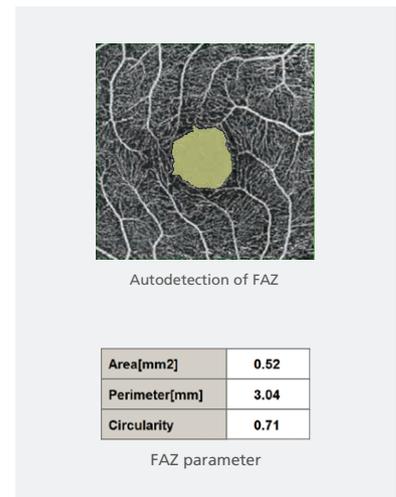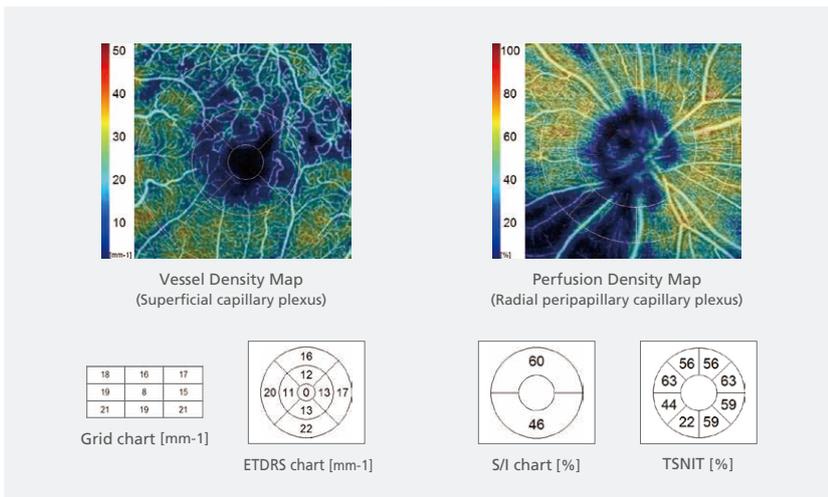

### Wide area scan

Scan size can range from 3 mm to maximum of 12 mm in 0.3 mm increments in 512 x 512 scans.



### Tracing HD plus


The tracing HD plus function tracks eye movements to maintain the same scan location on the SLO image for accurate image capture.

### Selectable definition

Two, four, or eight scans per line (2 HD, 4 HD, or 8 HD) can be selected.


Evaluate retinal structure and function simultaneously using combined OCT and Microperimetry images

Various OCT modalities can be registered with Microperimetry.

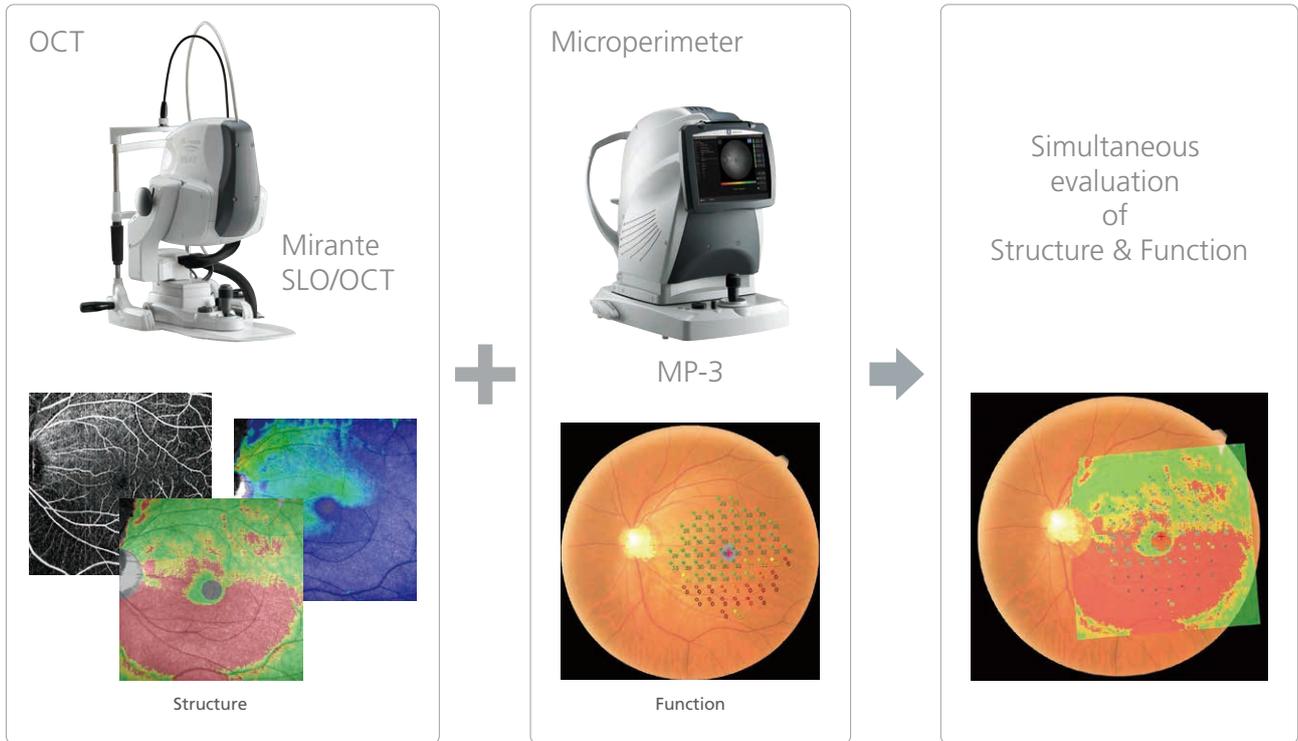


Clinical case

Age-related macular degeneration (AMD)

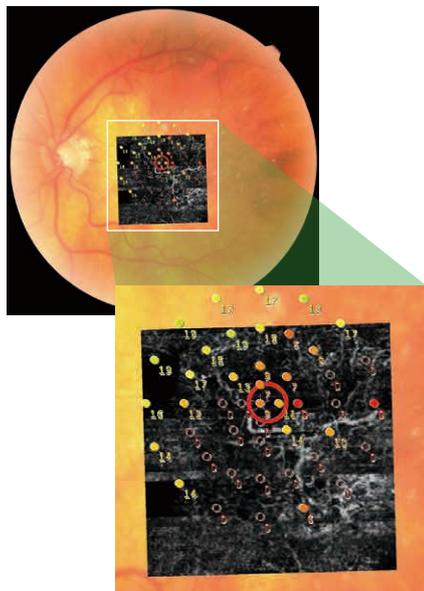

OCT-Angiography + Microperimetry (Outer retina)

Diabetic macular edema (DME)

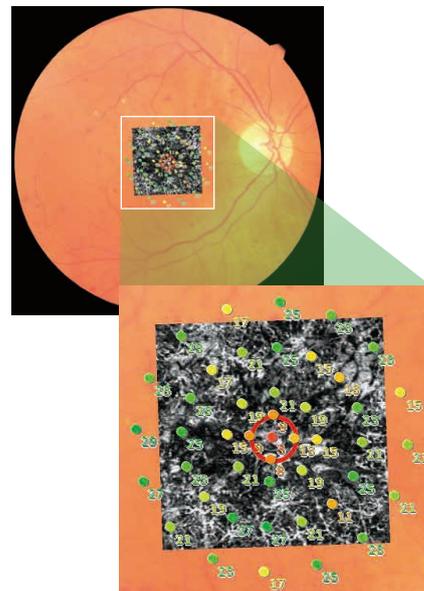

OCT-Angiography + Microperimetry (Deep capillary)

### Wide-field adapter


163° ultra wide field imaging is available with the optional wide-field adapter.



### Anterior segment OCT adapter\*


The optional anterior segment module enables observation and analyses of the anterior segment.

\* Available for the SLO/OCT model.

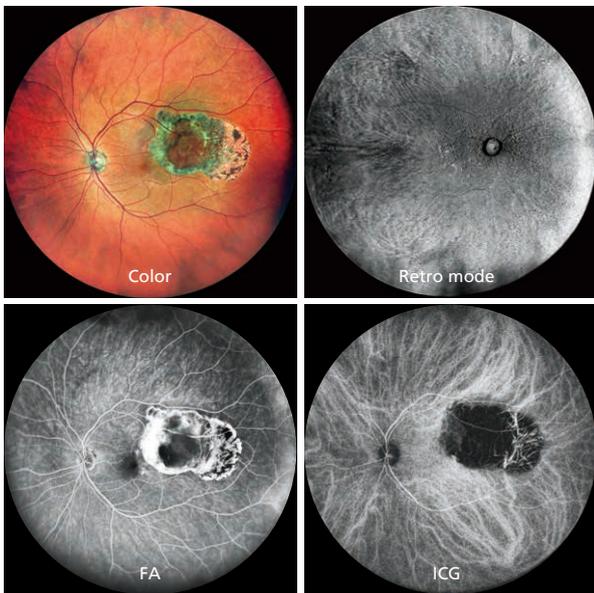



#### <Angle measurement>

- ACA
- AOD500 (AOD750)
- TISA500 (TISA750)

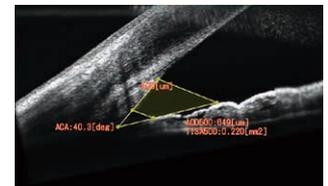

#### <Cornea measurement>



- Corneal thickness
  - Corneal apical thickness
  - user designated locations
- Corneal thickness map  
Map indicating corneal thickness plotted radially

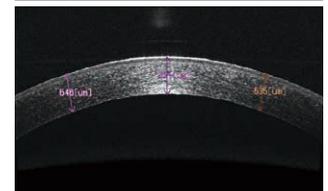

### Long axial length normative database


The long axial length normative database is optional software for assisting clinicians in diagnosing macular diseases and glaucoma in patients with long eyes. Data was collected from a sample of Asian patients.

Sample analysis of a patient with long axial length (27.0 mm)

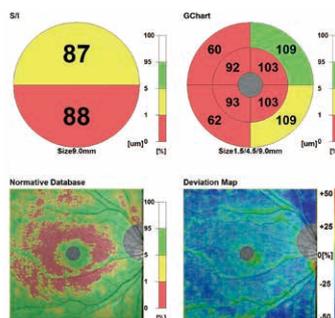

Normative database

Axial length compensation

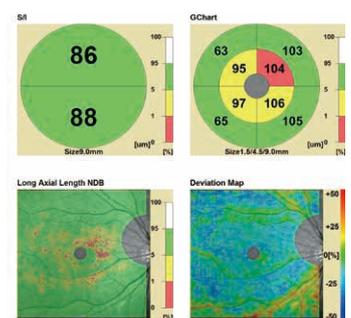

Long axial length normative database

# Function overview - Mirante and RS Series

●: Available

				Mirante SLO/OCT	Mirante SLO	RS-3000 Advance 2	Retina Scan Duo™ 2	
SLO/ Fundus image	Angle of view	Ultra wide field*1	163°*2	●	●			
		Standard	89°*2	●	●			
	Still image definition (pixel x pixel)	4,096 x 4,096		●	●			
		2,048 x 2,048		●	●			
		1,536 x 1,536		●	●			
		1,024 x 1,024		●	●			
		768 x 768		●	●			
		512 x 512		●	●			
	Color fundus	Color		●	●		●	
	Fundus fluorescence	FA/ICG		●	● (optional)*3			
	Fundus autofluorescence	Blue-FAF		●	●			
		Green-FAF		●	●		● (FAF model)	
	Retro mode	DR/DL/RA		●	●			
Red-free	RGB		●	●		●		
OCT	Scan speed	Up to 85,000 A-scans/s		●		●		
		Up to 70,000 A-scans/s					●	
	OCT sensitivity	Regular	85,000 A-scans/s		●		●	
			70,000 A-scans/s					●
		Fine	53,000 A-scans/s		●		●	●
			Ultra fine	26,500 A-scans/s				
		13,250 A-scans/s		●		●		
	A-scan	2,048 points		●				
		1,024 points		●		●	●	
		512 points		●		●	●	
		256 points		●		●	●	
	B-scan*4	256 scans		●		●	●	
		128 scans		●		●	●	
		64 scans		●		●	●	
		32 scans		●		●		
		16 scans		●		●		
	OCT-Angiography*5	512 x 512 scans		●				
		320 x 320 scans					●	
		256 x 256 scans		●		●		
		Tracing HD plus		●		●		
Scan range	X: 3 to 16.5 mm		●					
	X: 3 to 12 mm				●	●		
	Y: 3 to 13.2 mm		●					
	Y: 3 to 9 mm				●	●		
Scan wavelength	880 nm		●		●	●		

\*1 Ultra wide field imaging is available with the optional wide-field adapter.

\*2 Measured from the center of the eye

\*3 "FA only" option is also available.

\*4 Only for macula map and disc map

\*5 Optional

# Mirante Specifications

<b>SLO</b>	
Principal	Confocal scanning
Angle of view (Measured from the center of the eye)	Standard: Diagonal angle of view 89° Ultra wide field*1: $\phi$ 163°
Light source	488, 532, 670, 790 nm
Still image size	4,096 x 4,096, 2,048 x 2,048, 1,536 x 1,536, 1,024 x 1,024, 768 x 768, 512 x 512 (pixel x pixel)
Video size*2	1,024 x 1,024, 768 x 768, 512 x 512 (pixel x pixel)
Minimum pupil diameter	$\phi$ 3.3 mm
Working distance	Standard: 19 mm / Ultra wide field*1: 9 mm
<b>OCT*3</b>	
Principal	Spectral domain OCT
Optical resolution	Z: 7 $\mu$ m, X-Y: 20 $\mu$ m
Scan range	
Retina	X: 3 to 16.5 mm, Y: 3 to 13.2 mm, Z: 2.1 mm
Anterior*4	X: 2 to 8 mm, Z: 2.1 mm
OCT light source	SLD, 880 nm
Scan speed	Up to 85,000 A-scans/s
Image averaging	Up to 120 images
Normative database	9 x 9 mm (macula), 6 x 6 mm (disc)
Minimum pupil diameter	$\phi$ 2.5 mm
Working distance	Standard: 19 mm / Anterior*4: 15.4 mm
Software analysis	
Retina	Segmentation of 6+1 retinal layers, macular thickness map, RNFL thickness map, [NFL+GCL+IPL] analysis, optic nerve analysis
Anterior*4	Corneal thickness measurement, corneal thickness map, angle measurement
<b>Common specification</b>	
Diopter correction range	-15 to +15 D
Internal fixation lamp	Red (670 nm) / blue (488 nm)
External fixation lamp	White
Tilt	$\pm$ 10°
Swing	$\pm$ 20°
PC networking	Available
<b>Power supply</b>	100 to 240 V AC, 50/60 Hz
<b>Power consumption</b>	Device main body 150 VA
<b>Dimensions/mass*5</b>	345 (W) x 548 (D) x 527 to 557 (H) mm / 23 kg (SLO/OCT model) 22 kg (SLO model) 13.6 (W) x 21.6 (D) x 20.7 to 21.9 (H)" / 51 lbs. (SLO/OCT model) 49 lbs. (SLO model)
<b>Optional accessories</b>	Wide-field adapter, motorized optical table, PC rack, isolation transformer, external fixation lamp (multi-joint), anterior segment OCT adapter*3, AngioScan (OCT-Angiography)*3, long axial length normative database*3, B-Scan Denoising Software*3, FA/ICG dongle*6, FA dongle*6

\*1 Ultra wide field imaging is available with the optional wide-field adapter.

\*2 Optional for the SLO model.


\*3 Available for the SLO/OCT model.

\*4 Anterior segment OCT adapter is optional.


\*5 Only for image capturing unit.

\*6 Available for the SLO model.

## Central angle of view

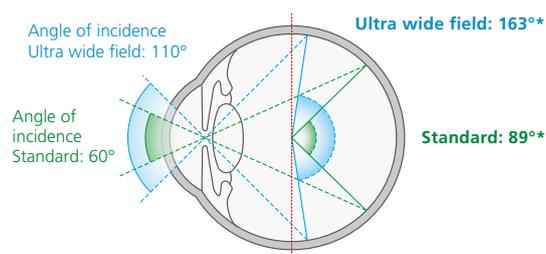

\* Measured from the center of the eye

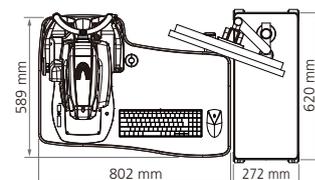

Images courtesy of

Luigi Sacco Hospital, University of Milan, Italy

Asia Eye Centre, Singapore

Doheny Eye Center, UCLA, USA

Retina Foundation & Eye Research Center, India

Kagoshima University Hospital, Japan

Exilaser Clinic, Peru

Chiba University Hospital, Japan

Tohoku University, Japan

Careggi University Hospital, University of Florence, Italy



**More clinical information available  
online at the NIDEK Education page**

For more clinical information, please visit the Education page on the NIDEK website. This site allows access to case reports, journal articles, and video presentations.



<https://www.nidek-intl.com/education/>

Product/model name: Scanning Laser Ophthalmoscope Mirante

Brochure and listed features of the device are intended for non-US practitioners.

Specifications may vary depending on circumstances in each country.

Specifications and design are subject to change without notice.

 Eye & Health Care  
**NIDEK CO., LTD.**

**HEAD OFFICE**  
(International Div.)  
34-14 Maehama,  
Hiroishi-cho, Gamagori,  
Aichi 443-0038, JAPAN  
TEL: +81-533-67-8895  
URL: www.nidek.com

**TOKYO OFFICE**  
(International Div.)  
3F Sumitomo Fudosan Hongo  
Bldg., 3-22-5 Hongo, Bunkyo-ku,  
Tokyo 113-0033, JAPAN  
TEL: +81-3-5844-2641  
URL: www.nidek.com

**NIDEK INC.**  
2040 Corporate Court,  
San Jose, CA 95131, U.S.A.  
TEL: +1-408-468-6400  
+1-800-223-9044  
(US Only)  
URL: usa.nidek.com

**NIDEK S.A.**  
Ecoparc,  
9 rue Benjamin Franklin,  
94370 Sucy En Brie,  
FRANCE  
TEL: +33-1-49 80 97 97  
URL: www.nidek.fr

**NIDEK TECHNOLOGIES S.R.L.**  
Via dell'Artigianato,  
6/A, 35020 Albignasego (Padova),  
ITALY  
TEL: +39 049 8629200/8626399  
URL: www.nidektechnologies.it

**NIDEK (SHANGHAI) CO., LTD.**  
Rm3205, Shanghai Multi  
Media Park, No.1027 Chang  
Ning Rd, Chang Ning District,  
Shanghai, CHINA 200050  
TEL: +86 021-5212-7942  
URL: www.nidek-china.cn

**NIDEK SINGAPORE PTE. LTD.**  
51 Changi Business Park  
Central 2, #06-14,  
The Signature 486066,  
SINGAPORE  
TEL: +65 6588 0389  
URL: www.nidek.sg

[Manufacturer]